

SUPPLEMENTARY MATERIAL

Application of Voltammetry in Biomedicine – Recent Achievements in

Enzymatic Voltammetry

Rubin Gulaboski¹, Valentin Mirceski^{2,3}

¹Faculty of Medical Sciences, "Goce Delcev" University, Stip, Macedonia

*²Faculty of Natural Sciences and Mathematics, Ss. Cyril and Methodius University, Skopje,
Macedonia*

*²Department of Inorganic and Analytical Chemistry, University of Lodz, Tamka 12, 91-403
Lodz, Poland*

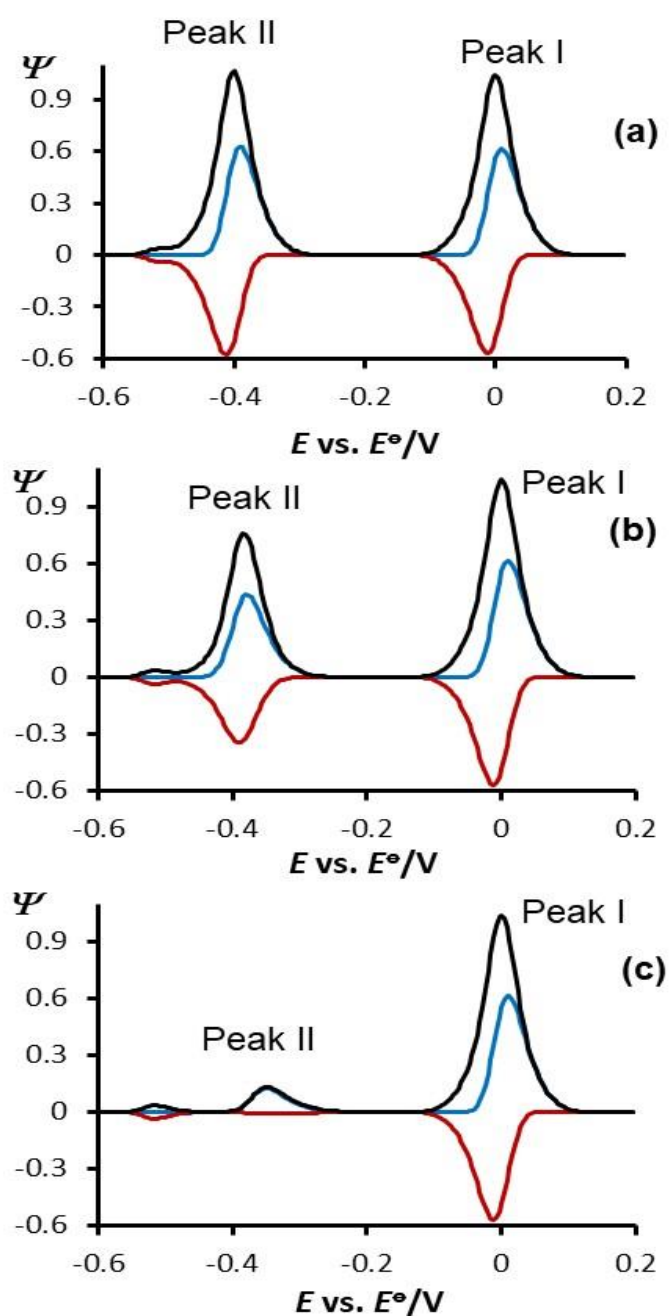


Figure S1. Surface EEC mechanism $A(\text{ads}) + n_1e^- \leftrightarrow B(\text{ads}) + n_2e^- \leftrightarrow C(\text{ads}) + S \leftrightarrow D(\text{ads})$ in protein-film voltammetry: effect of the substrate concentration $c(S)$ to the features of theoretical SW voltammograms. Voltammograms are simulated at potential separation of $|400 \text{ mV}|$ between both electrode steps: The values of $c(S)/\text{molL}^{-1}$ are set to: 0.0001 (a); 0.01 (b); and 0.05 (c). The value of chemical rate constant was set to $k_{\text{chem}} = 10 \text{ mol}^{-1}\text{Ls}^{-1}$. Equilibrium constant of follow-up chemical reaction was $K_{\text{eq}} = 1000$. All other simulation parameters were same as those in figure 3.

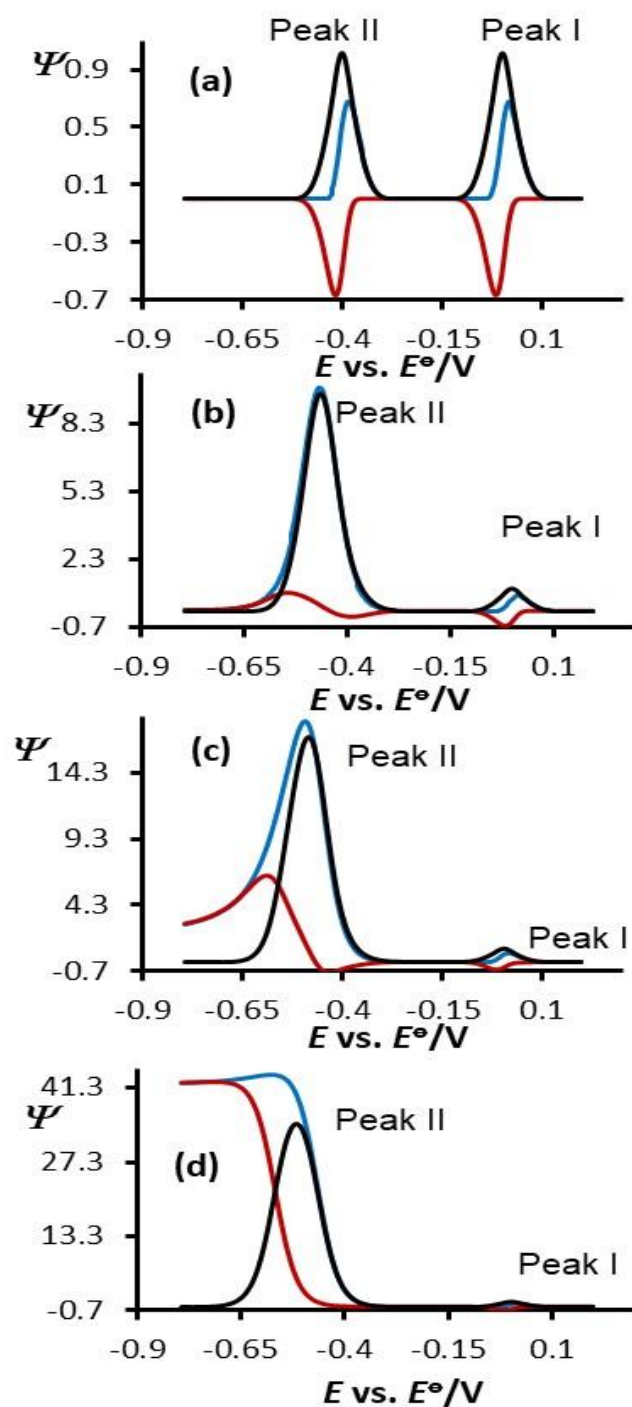


Figure S2. Surface EEC' regenerative mechanism $A(\text{ads}) + n_1e^- \leftrightarrow B(\text{ads}) + n_2e^- \leftrightarrow C(\text{ads}) + S \rightarrow B(\text{ads})$ in protein-film voltammetry: effect of the substrate concentration $c(S)$ to the features of theoretical SW voltammograms. Values of $c(S)/\text{molL}^{-1}$ are set to: 0.0001 (a); 0.03 (b); 0.035 (c) and 0.05 (d). The value of catalytic rate constant was set to $k_c = 10 \text{ mol}^{-1}\text{Ls}^{-1}$. All other simulation parameters were same as those in figure 3.